

IMPLANT WITH PRESSURE SENSOR FOR GLAUCOMA TREATMENT

Morteza Gharib, et al.

Appl. No.: Unknown Atty Docket: GLAUKO.005C1

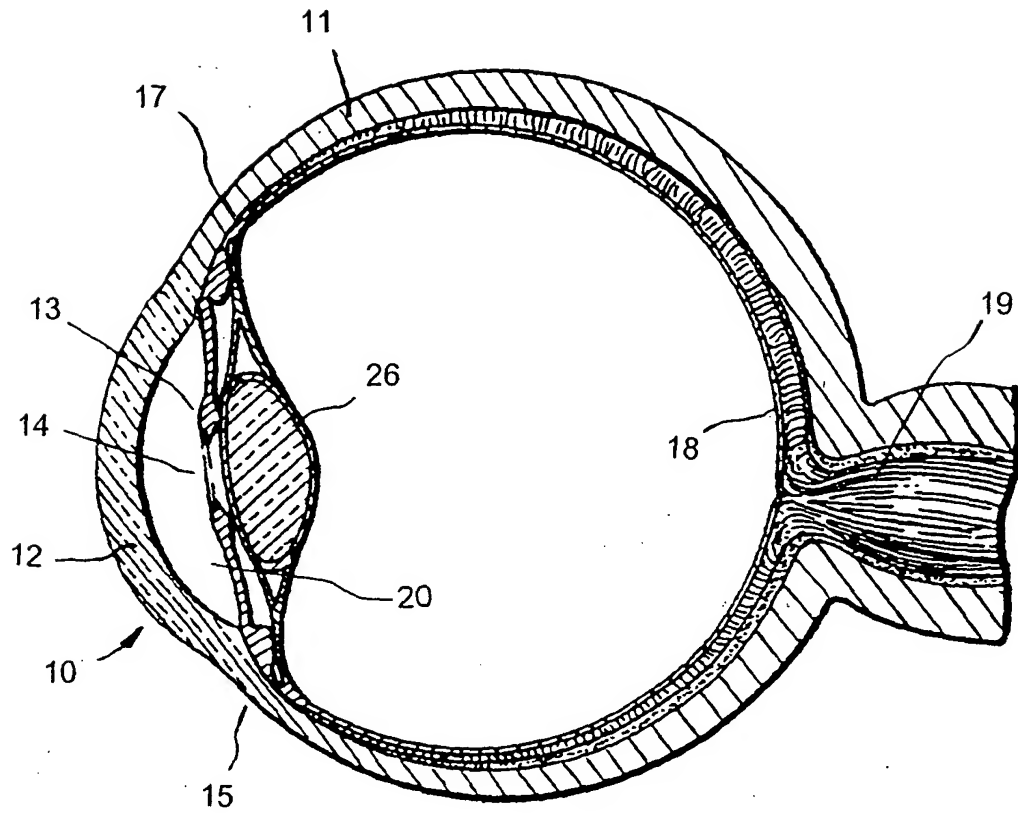


FIG. 1

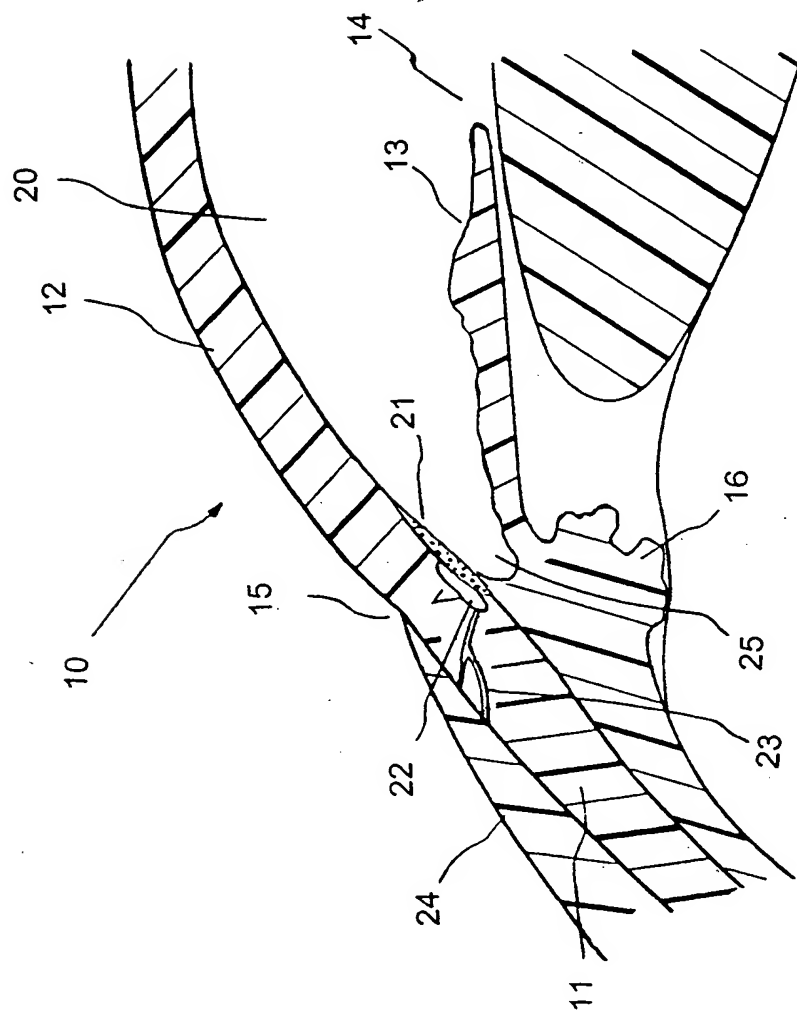


FIG. 2

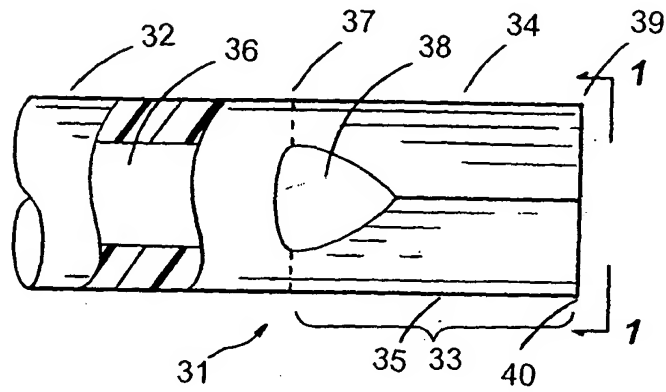


FIG. 3A




FIG. 3B

Appl. No.: Unknown Atty Docket: GLAUKO.005C1



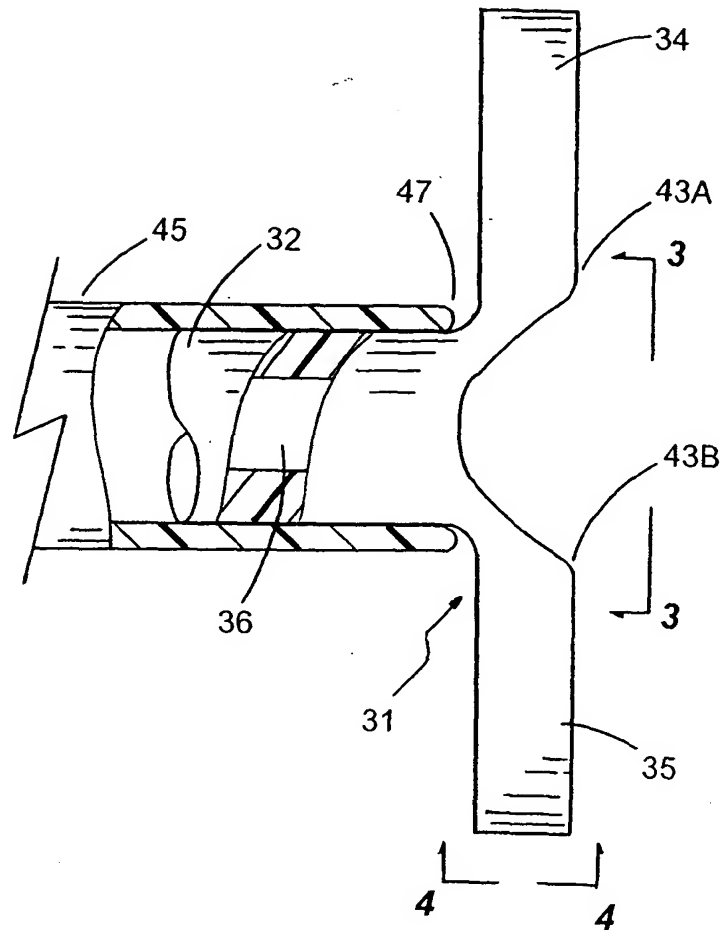


FIG. 5A

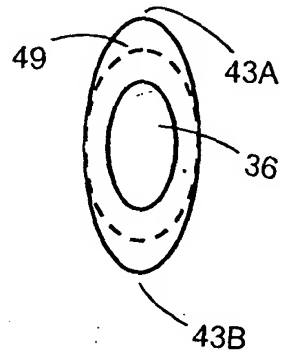


FIG. 5B




FIG. 5C

IMPLANT WITH PRESSURE SENSOR FOR GLAUCOMA TREATMENT

Morteza Gharib, et al.

Appl. No.: Unknown

Atty Docket: GLAUKO.005CI

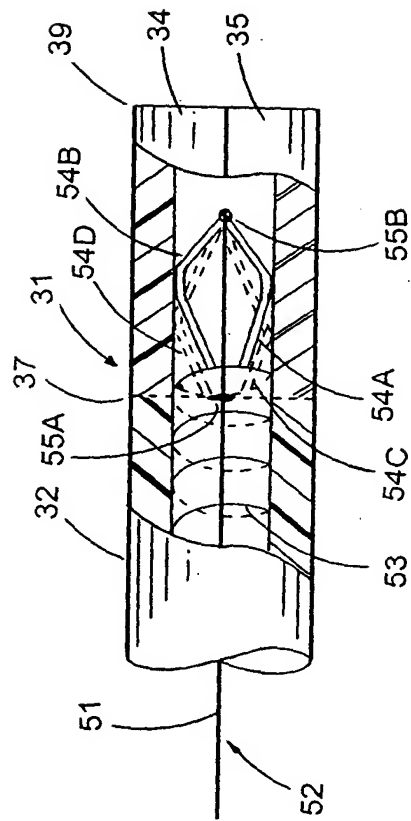


FIG. 6

IMPLANT WITH PRESSURE SENSOR FOR GLAUCOMA TREATMENT

Morteza Gharib, et al.

Appl. No.: Unknown Atty Docket: GLAUKO.005C1

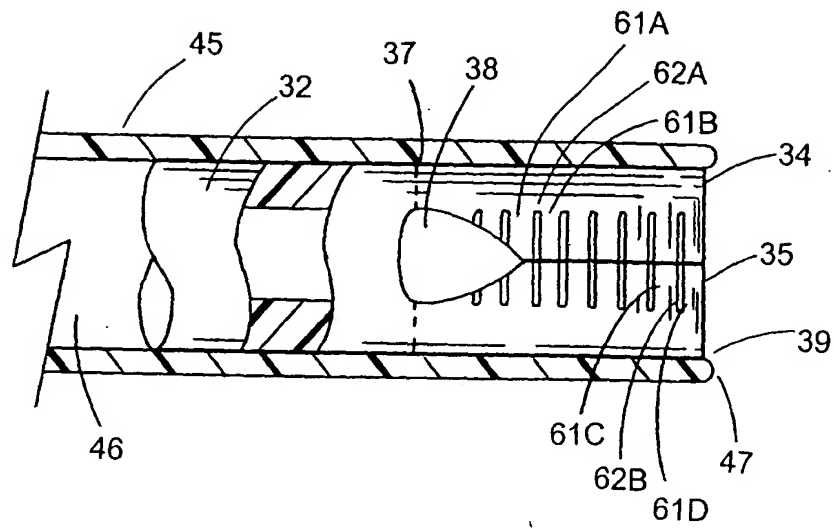


FIG. 7A

IMPLANT WITH PRESSURE SENSOR FOR GLAUCOMA TREATMENT

Morteza Gharib, et al.

Appl. No.: Unknown Atty Docket: GLAUKO.005C1

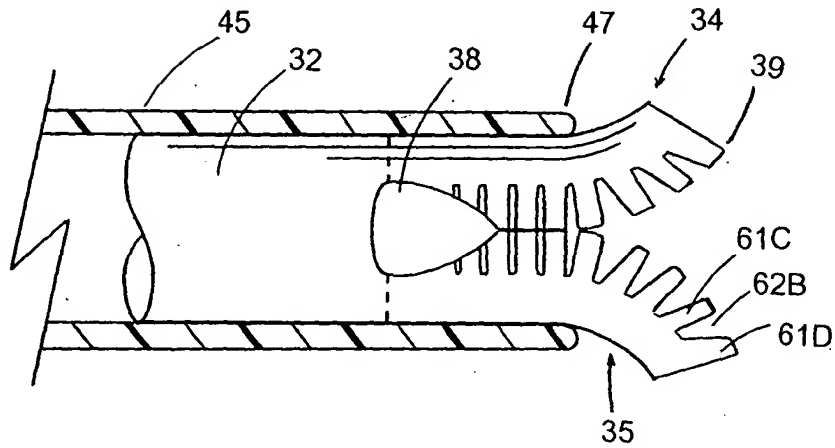


FIG. 7B

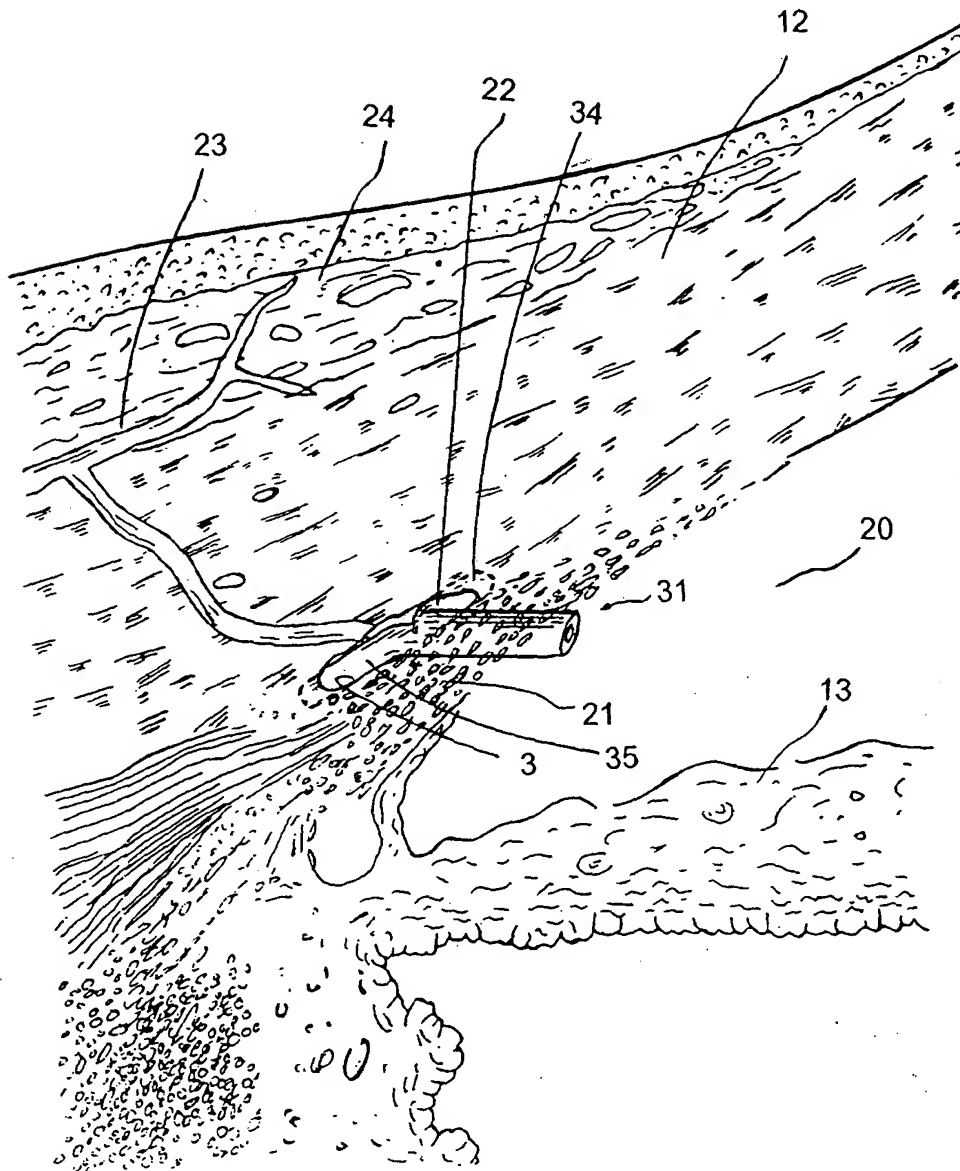


FIG. 8